FIG. 1

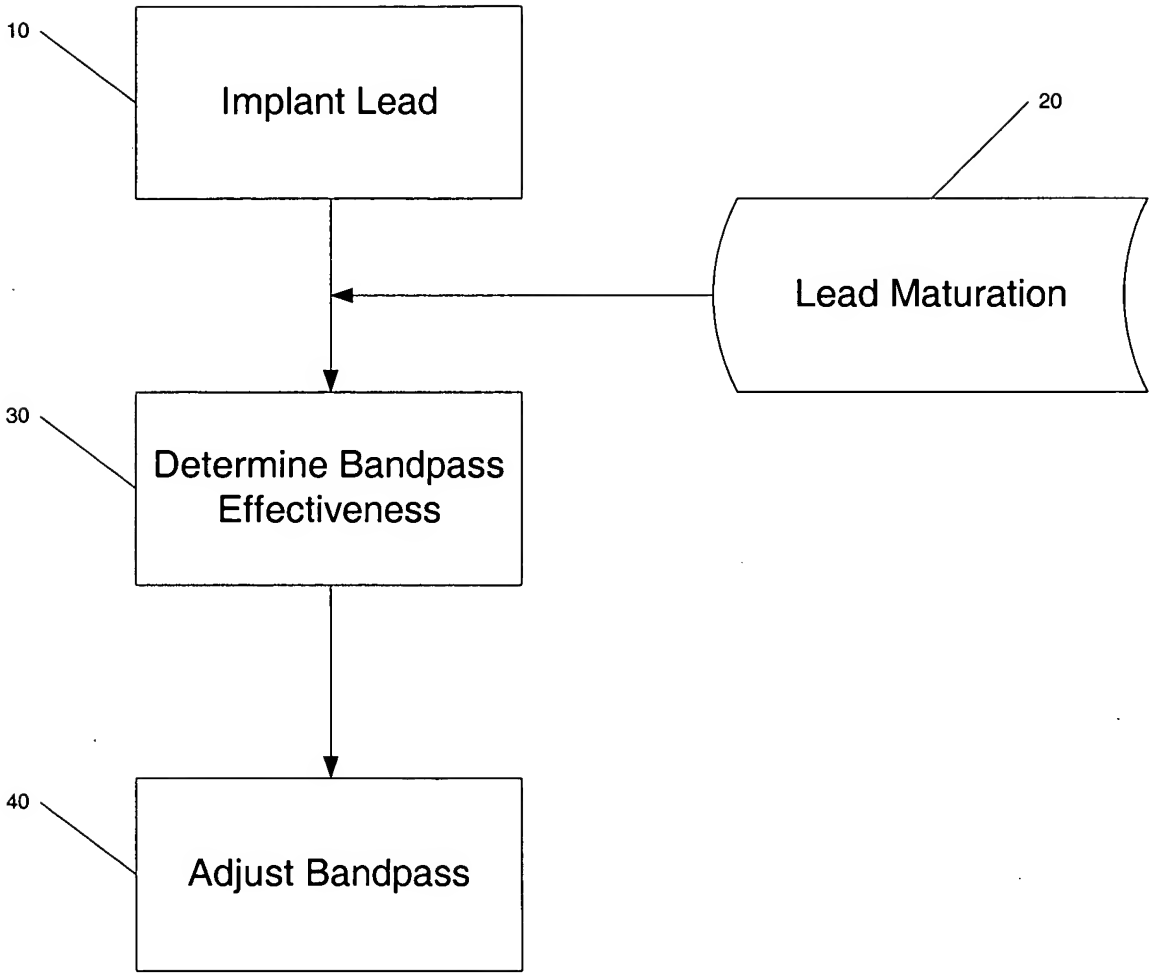
10
Implant Lead
20
Lead Maturation
30
Determine Bandpass Effectiveness
40
Adjust Bandpass